

Fitness, body weight loss and inappropriate shocks of subcutaneous-implantable cardioverter-defibrillator – a case report

Diana Paskudzka^{1,A-F}, Agnieszka Kołodzińska^{1,A-F}, Łukasz Januszkiewicz^{1,A-F}, Marcin Grabowski^{1,E-F}

A - Research concept and design, B - Collection and/or assembly of data, C - Data analysis and interpretation, D - Writing the article, E - Critical revision of the article, F - Final approval of article

1 Medical University of Warsaw

Address for correspondence:

Dr. Diana Paskudzka, Medical University of Warsaw
email: paskudzkadiana@gmail.com

Dr. Agnieszka Kołodzińska, Medical University of Warsaw
email: aa.kolodzinska@wp.pl

Dr. Łukasz Januszkiewicz, Medical University of Warsaw
email: lukasz.jan.januszkiewicz@gmail.com

Prof. Marcin Grabowski, Medical University of Warsaw
email: marcin.grabowski@wum.edu.pl

Received: 2020-09-15

Revised:

Accepted: 2021-02-08

Final review:

DOI: 10.24255/hbj/133171

Key words:

S-ICD, shock, inappropriate shock, Physical Exercises

Abstract

The subcutaneous implantable cardioverter-defibrillator (S-ICD) is a well-established method for the prevention of sudden cardiac arrest and an alternative to the transvenous implantable cardioverter-defibrillator (TV-ICD). It is preferred mainly for young patients with long life expectancy, high risk of transvenous lead complications or a history of previous

endocarditis, or device infections. For both S-ICD and TV-ICD, inappropriate therapies are possible. For S-ICD, the most common cause of inappropriate shocks is T wave oversensing (TWOS), while in TV-ICD it is supraventricular tachycardia. We present the case of a 38-year-old patient who reported a shock during physical exercise – sit-ups.

Introduction

The S-ICD is an established therapy for prevention of sudden cardiac death and an alternative to TV-ICD in selected patients. These types of devices are especially recommended for young patients with long life expectancy, lack of venous access for TV-ICD implantation or high risk associated with leads or history of previous endocarditis or device infections. The first S-ICDs were introduced in 2009. Since then, improvements have been made to reduce the device's size, increase battery life and upgrade detection algorithms to prevent inappropriate shocks⁽¹⁾. The rate of inadequate shocks ranges from 4 to 25%, and it is similar to a TV-ICD 20-30%. However, the mechanism

is different. For S-ICD, up to 80% are caused by TWOS, particularly in selected patient populations (i.e. congenital heart disease, Brugada and long QT syndrome). In intravenous devices, TWOS are responsible for up to 20% of cases⁽²⁻⁵⁾. In the case of high risk of TWOS, it is worth considering performing an exercise test after the implantation to properly program the sensory vector⁽⁶⁾. Changing the sensitivity of the device and sensing vector often helps to solve the problem⁽⁷⁾. In addition, about 5 to 10% of the inappropriate shocks can be caused by noise related to myopotential oversensing⁽⁴⁾. For an TV-ICD, the most common cause of inappropriate discharges is supraventricular tachycardia⁽⁸⁾.

Case report

A 38-year-old man with an implanted S-ICD visited the ambulatory clinic of implantable devices due to a shock of the device a few days earlier. The patient had a history of: implantation of S-ICD in secondary prevention (2017), dilated cardiomyopathy, chronic heart failure in NYHA class II, paroxysmal atrial fibrillation, pulmonary vein isolation (2019), and obesity. Since cardiac arrest the patient has changed his lifestyle dramatically, started regular physical activity and lost about 20 kg. Being in good general condition, without signs of exacerbation of heart failure, a few days ago the patient had got a shock. The patient did not lose consciousness. There were no prodromal symptoms.

The current follow-up revealed an episode detected by the device as ventricular fibrillation and then a high-energy discharge. The shock zone was programmed from 220 bpm and the conditional shock zone from 200 bpm. Battery status was 64%. On the basis of the recording from the device it was difficult to clearly determine whether it was an artifact or an inappropriate shock (Figure 1). The patient stated that

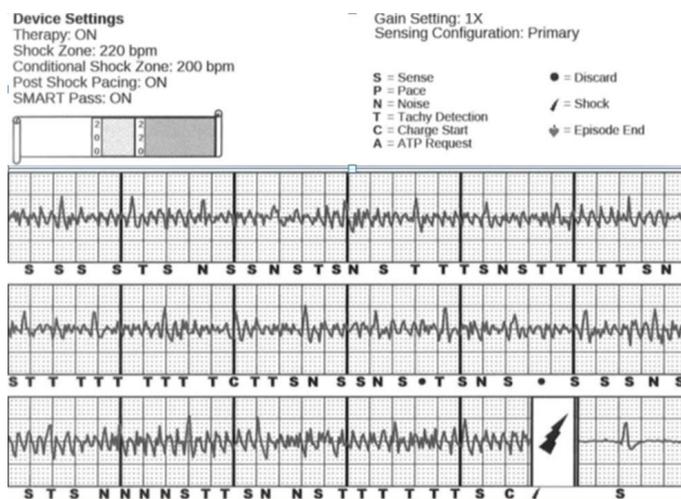


Figure 1.

he was doing physical exercise – sit ups – when the shock occurred. Therefore, a provocative test was performed in the laboratory. The patient was asked to lie down on the couch and perform exercises such as during the episode. The myopotential oversensing of the device during the exercise was confirmed (Figure 2). The patient was advised to avoid such and similar exercises.



Figure 2.

References

1. Kaya E, Rassaf T, Wakili R. Subcutaneous ICD: Current standards and future perspective. *Int J Cardiol Heart Vasc.* 2019; 24: 100409.
2. Aydin A, Hartel F, Schlüter M, et al. Shock efficacy of subcutaneous implantable cardioverter-defibrillator for prevention of sudden cardiac death: initial multicenter experience. *Circ Arrhythm Electrophysiol* 2012; 5(5): 913-9.
3. Köbe J, Reinke F, Meyer C, et al. Implantation and follow-up of totally subcutaneous versus conventional implantable cardioverter defibrillators: a multicenter case-control study. *Heart Rhythm* 2013; 10(1): 29-36.
4. Olde Nordkamp LR, Dabiri Abkenari L, Boersma LV, et al. The entirely subcutaneous implantable cardioverter-defibrillator: initial clinical experience in a large Dutch cohort. *J Am Coll Cardiol* 2012; 60(19): 1933-9.
5. Jarman JW, Todd DM. United Kingdom national experience of entirely subcutaneous implantable cardioverter-defibrillator technology: important lessons to learn. *Europace* 2013; 15(8): 1158-65.
6. Kooiman KM, Knops RE, Olde Nordkamp L, et al. Inappropriate subcutaneous implantable cardioverter defibrillator shocks due to T-wave oversensing can be prevented: implications for management. *Heart Rhythm* 2014; 11(3): 426-34.
7. Corzani A, Ziacchi M, Biffi M, et al. Inappropriate shock for myopotential over-sensing in a patient with subcutaneous ICD. *Indian Heart J.* 2015;67(1):56-59.
8. De Maria E, Oлару A, Cappelli S. The entirely subcutaneous defibrillator (s-icd): state of the art and selection of the ideal candidate. *Curr Cardiol Rev.* 2015; 11(2): 180-186.